



Review

Oxygen devices and delivery systems

Cite as: Hardavella G, Karampinis I, Frille A, *et al.* Oxygen devices and delivery systems. *Breathe* 2019; 15: e108–e116.

Oxygen use has extended from inpatient to outpatient settings for patients with chronic pulmonary diseases and complications of hypoxaemia. This article presents an overview of oxygen devices (oxygen concentrators, compressed gas cylinders and liquid oxygen) and delivery systems (high- and low-flow). The indications, advantages and disadvantages of each device and delivery system are presented, aiming to offer updated knowledge to the multidisciplinary team members managing patients with respiratory failure, and therefore allowing appropriate selection of devices and delivery systems that are tailored to the needs of each patient.

Introduction

Oxygen use has extended from inpatient to outpatient settings for patients with chronic pulmonary diseases and complications of hypoxaemia. The Nocturnal Oxygen Trial and a study published by the British Medical Research Council are the landmark studies that have consolidated evidence for domiciliary oxygen use [1, 2]. The following three groups of patients with chronic hypoxaemic lung diseases are suitable for long-term oxygen therapy (LTOT) [3, 4]:

- 1) Patients with arterial oxygen tension (P_{aO_2}) ≤ 55 mmHg at rest in nonrecumbent position, despite optimal treatment of underlying condition.
- 2) Patients with $P_{aO_2} > 55$ mmHg associated with evidence of central nervous system dysfunction, cor pulmonale, secondary pulmonary hypertension or polycythaemia.

- 3) Patients with demonstrable fall in P_{aO_2} below 55 mmHg and desaturation during sleep and/or exercise.

Nowadays, LTOT use is higher in women, and this is projected to increase further in the near future due to the high number of middle-aged female smokers [5]. There is a large variety of available oxygen-conserving devices and, considering the high costs of LTOT and the impact on patients' health-related quality of life, optimal device selection and prescribing requires a clear understanding of these devices [3, 6–8]. In this review, we will present different oxygen devices and delivery systems.

Oxygen concentrators

How do they work?

Oxygen concentrators provide a safe source of oxygen-enriched air. Oxygen concentrators



CrossMark



© ERS 2019



@ERSpublications

Consolidated knowledge of all oxygen devices and delivery systems is essential to devise tailored patient-based plans for oxygen therapy <http://bit.ly/2kh5f2G>

(sometimes referred to as oxygen generators) are devices that draw room air through a series of filters that remove dust, bacteria and other particulates. In the first step of the concentration process, the machine forces air into one of the two cylinders containing a molecular “sieve” material or semi-permeable membranes, where nitrogen is absorbed, leaving concentrated oxygen (90% or higher) and a small percentage of other gases found in room air. At the same time, in the other cylinder, nitrogen is desorbed and drawn out into the atmosphere. In the second step, the function of the cylinders is reversed in a timed cycle, providing a continuous flow of oxygen to the patient. A typical oxygen concentrator may deliver oxygen flows of 0.5–5 L·min⁻¹ (low-flow oxygen concentrators), while some models may generate up to 10 L·min⁻¹ (high-flow oxygen concentrators) [9, 10].

Types of oxygen concentrators and oxygen delivery

There are two types of oxygen concentrators: stationary and portable [9, 10]. Stationary (home) concentrators provide an uninterrupted oxygen supply with a flow ranging from 0.5 to 10–15 L·min⁻¹. They have a mean weight of about 10 kg. They have several ergonomic handles built in, to offer options for lifting or rolling the device (figure 1a). New miniature concentrators have recently entered the market, making stationary concentrators more mobile than ever. The concentrator plugs into the main electricity supply at home, using 300 W (or below) per hour (about the same as four light bulbs). A back-up compressed gas cylinder is sometimes provided, to use in case of a power failure.

A relatively new option is a super small home concentrator, which can weigh approximately 4.5 kg. These units run on both alternating current (AC; *e.g.* from a wall socket) and direct current (DC; *e.g.* from a cigarette lighter socket) and are mobile (*e.g.* they can be easily moved from one room to the other or they can be transported by car for travel). They currently support oxygen flow rates up to 2 L·min⁻¹.

Portable oxygen concentrators are the latest technology for LTOT users who desire a small, lightweight and portable oxygen solution in a compact and mobile unit (figure 1b). Portable concentrators vary in weight, size, oxygen flow settings, range of L·min⁻¹ and battery life, as well as other specifications.

The key differences between stationary and portable concentrators can be summarised by four major factors: 1) oxygen output, 2) size and weight, 3) power options and 4) price. Stationary oxygen concentrators have higher oxygen output and lower costs. Portable oxygen concentrators offer smaller size and less weight as well as greater flexibility with power sources. For patients who live active lives and are often away from an AC (wall socket) power source, a portable oxygen concentrator

is the best choice [9, 10]. Most portable oxygen concentrators use lithium ion batteries, which degrade over time. Most of these batteries can be recharged approximately 300 times without significant degradation.

Generally, there are two types of oxygen delivery in oxygen concentrators: continuous flow dose delivery and pulse mode delivery. Continuous flow dose delivery supplies a constant, steady and reliable oxygen flow based on the setting number in L·min⁻¹, while pulse mode delivery delivers a pulsed “bolus” of oxygen when the user begins to take a breath. Initially, the individual flow setting should be adjusted.

Indications

Stationary oxygen concentrators are commonly used by patients on LTOT, as they are cost-effective and are safer than using compressed gas cylinders. Oxygen concentrators are recommended for patients using oxygen for >1.4 h·day⁻¹ [10]. Guidelines do not give indications for the choice of the delivery device but only suggest the use of a portable device in subjects on LTOT who regularly go outside [9]. Portable oxygen concentrators for ambulatory oxygen therapy are offered to people already on LTOT who want to use oxygen outside the home. Ambulatory oxygen therapy can improve exercise tolerance and breathlessness, although there is no benefit from oxygen before and after exercise in most patients with chronic obstructive pulmonary disease (COPD). Furthermore, ambulatory oxygen therapy may allow increased daily oxygen use and/or better compliance.

Advantages and disadvantages

Evidence arising from both prospective and retrospective trials and randomised controlled trials (with a minimum 12-month follow-up) suggests that oxygen concentrator use where appropriate improves

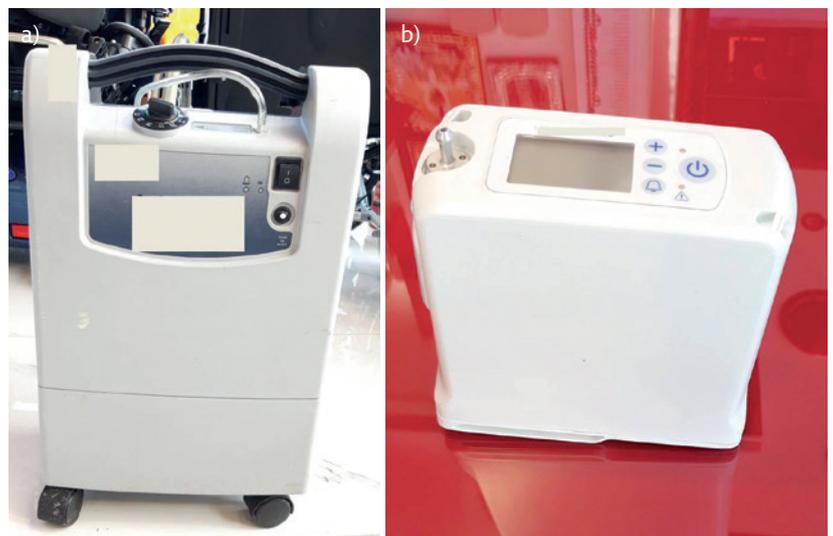


Figure 1 a) Stationary oxygen concentrator. b) Portable oxygen concentrator.

survival rates for respiratory conditions, improves mental attentiveness, increases stamina and improves mood. The majority of studies have been performed in patients with COPD and it is of note that the duration of oxygen supply *per se* affects survival. In hypoxaemic chronic obstructive lung disease, continuous oxygen therapy is associated with a lower mortality than is nocturnal oxygen therapy [1–5].

Advantages

Oxygen concentrators do not need to be refilled. The concentrators run on electrical power and thus supply an unlimited amount of oxygen. Portable concentrators can be used in an “on-the-go” mode with a battery pack, resulting in up to 12 h of continuous use for some models. From a long-term view, concentrators are more cost-effective than compressed gas cylinders, and they are known to last for up to 1500 h of continuous use [11, 12].

Disadvantages

The significant disadvantage of oxygen concentrators is the need for electrical power to function. It is necessary to prepare for unscheduled power outages by setting up a backup power generator at home. Patients using stationary oxygen concentrators need to consider changing filters weekly, regular servicing and the warm-up period of the machine, as well as noise and vibration from the older models of device [11, 12].

Related costs

The global market for medical oxygen concentrators was valued at USD 1.75 billion in 2018 [13]. The market is anticipated to expand at a compound annual growth rate of 7.4% between 2019 and 2025 [13]. The prices of new home oxygen concentrators depend on batteries and other

accessories, and range from USD 595 to USD 2000. Used oxygen concentrators are cheaper (USD 595–1500), depending on the hours, warranty, and condition of the unit. However, the rental of a stationary oxygen concentrator can run from USD 35 per day to over USD 200 per week, but extended rental contracts may allow for a discount [13].

Compressed gas cylinders

Compressed gas cylinders have certain differences when compared to oxygen concentrators, and these are summarised in table 1. Figure 2a shows a compressed gas cylinder and figure 2b shows a patient in bed receiving oxygen from it *via* a nasal cannula.

Properties, classification and appearance

A cylinder is a metal container filled with compressed gas and held under high pressure. Oxygen cylinders are available in a range of sizes that determine the capacity for oxygen. For compressed oxygen cylinders, there are three methods of delivering portable oxygen: a portable cylinder, lightweight cylinder, and home fill cylinder [14]. When fully filled with oxygen, cylinders range from small portable cylinders for ambulatory use (*e.g.* 53 cm height, 3 kg weight, 430 L of oxygen) to large static cylinders (*e.g.* 71 cm height, 18 kg weight, 2122 L of oxygen) [14]. A backpack, trolley or wheeled cart may be necessary for locomotion, depending on cylinder size and weight as well as the patient's activity and fitness level. The oxygen cylinders are colour coded with a white body to distinguish them from other medical gases.

How do they work?

A regulator is attached to the cylinder's top and works like a tap, allowing the safe adjustment

Table 1 Differences between oxygen concentrators and compressed gas cylinders

| | Oxygen concentrators | Compressed oxygen cylinders |
|----------------------------------|---|---|
| Power source required | Yes, continuously (according to model: 100–600 W) | No |
| Transport required | Only at the time of installation | Yes, regularly; heavy and costly to transport |
| Exhaustible oxygen supply | No, continuous supply as long as power remains uninterrupted | Yes, depending on the size, storage pressure, and patient needs |
| User care | Moderate: cleaning of filters and device exterior, and minimise fire hazard | Minimal: regular checking, minimise fire hazard (no grease or flammables) |
| Operational costs | Small: electricity and maintenance | High: cylinder refills and transport from refilling station to a hospital |
| Maintenance | Moderate: check for low oxygen output with analyser | Moderate: check for pressure leaks with gauge |

of oxygen flow rate provided, in $\text{L}\cdot\text{min}^{-1}$. When the tap is manually opened, the oxygen takes the line of least resistance to the patient *via* an oxygen delivery device (*e.g.* tube with a mask or nasal cannula). A pressure reading (barometer) displays the remaining oxygen pressure in the cylinder, to estimate the amount of oxygen available for supply.

The capacity of a compressed oxygen cylinder is comparatively low: *e.g.* with 200 bar filling pressure and 400 L of oxygen, the patient's oxygen supply will suffice for 2.5 h, depending on flow rate [15].

At home or in the hospital, cylinders are changed by the gas provider. The frequency of deliveries depends on the cylinder's size and oxygen consumption. Home fill cylinders can be refilled by an oxygen concentrator [14].

Compared to continuous oxygen flow, oxygen-conserving devices deliver pulsed oxygen during inspiration only, triggered by the patient's inspiration. These "demand" oxygen delivery systems enable cylinders to last longer, since the oxygen waste during expiration is reduced. It has been shown that conservers can reduce oxygen usage by 50%, leading to a reduced number of home deliveries and thus lower costs [14, 15]. However, oxygen-conserving devices vary in their ability to maintain arterial oxygen saturation levels during exercise, and some patients struggle to trigger them due to the advanced stage of their lung disease [14].

Indications

For patients requiring supplemental oxygen at home, compressed gas cylinders are commonly combined with an oxygen concentrator. These patients are less mobile, spend the majority of time at home and are rarely in need of mobile oxygen, which is why compressed gas cylinders may serve as a back-up if a power cut or concentrator failure occurs [14, 15].

In hospital, mobile compressed gas cylinders find their main use as a temporary oxygen supply for invasively ventilated patients when they need to undergo diagnostic or therapeutic procedures outside the intensive care unit [14, 15].

Correlation with clinical outcomes

When standard portable cylinders were compared with lightweight cylinders in patients with COPD, in a prospective, randomised, clinical, multicentre trial conducted by the COPD Clinical Research Network, no differences were found in activity levels, oxygen saturation, Borg score or 6-min walk test [16].

A randomised multi-arm repeated-measures prospective study compared the use of liquid oxygen, home fill cylinder, portable concentrator and lightweight cylinder in 39 patients with stable severe COPD. There were no differences



Figure 2 a) Compressed gas cylinder with an attached flowmeter, and b) a patient receiving oxygen from this device.

between oxygen saturation, distance walked, or time used [14, 17]. Another prospective, randomised clinical study performed in COPD patients compared liquid oxygen and cylinders for domiciliary portable use and found that neither of them improved the quality of life [18].

Advantages and disadvantages

Advantages

Nowadays, compressed oxygen cylinders are comparatively the least convenient oxygen supply modality. However, depending on the demand of the patient, a cylinder may suffice in combination with a stationary oxygen concentrator [14].

Disadvantages

Due to their size and weight, cylinders are less convenient to carry without equipment. Patients can benefit from the provision of trolleys, wheeled carts or backpacks to enable them to carry home oxygen equipment [14]. When compared to liquid oxygen, cylinders were least favoured, while liquid oxygen was most favoured, with the lowest long-term costs [14, 15]. Despite the lack of improvement in the quality of life, patients using portable cylinders, in comparison with liquid oxygen, spent significantly shorter periods outside the house and used their oxygen less [18].

Case presentation

A 90-year-old female patient from a nursing home presented at the emergency department due to acute onset of shortness of breath, cough and purulent sputum for the past few days. She denied fever and night sweats. She reported that she is a heavy smoker (80 pack-years of cigarettes) and has not been leaving the bed lately due to the deterioration of her COPD. So far, she had not

been in need of supplementary oxygen. Initial arterial blood gas testing showed hypoxaemia (P_{aO_2} 50 mmHg) without hypercapnia (P_{aCO_2} 40 mmHg) and with normal pH (7.40). Chest radiography was unremarkable except for signs of bilateral apical emphysema.

She was admitted for an acute exacerbation of COPD. After treatment with bronchodilators, intravenous corticosteroids, antibiotics, and oxygen *via* nasal cannula, she recovered quickly, within 5 days. Only the hypoxaemia did not improve back to normal limits without nasal oxygen supply. Since 2 L·min⁻¹ nasal oxygen fully resolved hypoxaemia (P_{aO_2} 70 mmHg) without developing hypercapnia, she was prescribed nasal oxygen supply.

After exhaustive discussion with her about her present needs at the nursing home, we decided to prescribe her an oxygen concentrator in combination with a compressed oxygen cylinder. With the help of the oxygen concentrator she would be supplied with oxygen in her room. The compressed oxygen cylinder would supply her with mobile oxygen when she needed to leave her room (*e.g.* when her family members visit her or she has a medical appointment outside the premises).

Liquid oxygen

The introduction of liquid oxygen transformed the landscape of domiciliary oxygen therapy [12]. The first home-based liquid oxygen system was developed in 1965 with the view of providing a larger stationary oxygen system inside the home, with smaller liquid oxygen portables that can be refilled and used outside the home [19, 20].

How do liquid oxygen systems deliver oxygen?

Liquid oxygen is a cryogenic liquid, that is, a liquefied gas with a boiling point of -183°C [21–23]. Liquid oxygen allows a larger quantity of oxygen (gas) to be stored as a liquid in a small receptacle [24]. The 860:1 expansion ratio for liquid oxygen means that when 1 L of liquid oxygen is evaporated, it expands to approximately 860 L of gaseous oxygen [25]. The medical liquid oxygen (minimum 99.5% purity) must first be vaporised to a compressed gas then warmed at ambient (room) temperature inside the equipment before the patient can receive the oxygen through tubing into the nostrils *via* a nasal cannula [22]. How long a patient can use the ambulatory oxygen in the portable flask depends on the flow rate of oxygen the patient is using, as prescribed by the treating physician [21].

Both the stationary storage containers (“mother unit vessels”) and portables come in different sizes. These cryogenic containers keep the liquid cold [24]. Small stationary containers may provide a convenient refill supply in a car or van during extended

trips from home [25]. If the patient is on high-flow liquid oxygen (up to 15 L·min⁻¹ of continuous flow oxygen), it is important to note that ice may form on the portable’s heat exchange coils due to freezing of ambient humidity [25]. These patients usually possess two portable systems to facilitate continuous usage, allowing for de-icing of one of the units while using the ambulatory oxygen in the other [25].

Indications

Selecting the right oxygen delivery system for the right candidate can be challenging for the clinician. There are two major deciding factors when choosing between liquid oxygen and oxygen from a compressed gas cylinder, which are convenience and efficiency. For ambulatory patients who wish to be mobile, limited French data from the ANTADIR registry support the use of portable liquid oxygen in this group [26]. According to the literature, liquid oxygen may be suitable for patients with chronic respiratory disabilities who could return to work, require flow rates >5 L·min⁻¹, can walk, and cannot carry out their activities without an oxygen supply [12, 18]. For ambulatory patients requiring high-flow oxygen, liquid oxygen is the most practical option [25]. Figure 3 shows a patient with a nasal cannula and liquid oxygen tank.

Correlation with clinical outcomes

Patients using liquid oxygen are more apt to venture outside the home and use daily oxygen for longer periods compared with their counterparts using



Figure 3 Patient with a nasal cannula and liquid oxygen tank.

oxygen concentrators [27]. In addition, liquid oxygen therapy improves both patient compliance and health-related quality of life [18, 28]. Significant differences, favouring liquid oxygen therapy *versus* oxygen concentrators, have been found in the following quality of life measures: physical function, body care, ambulation, social interaction and total Sickness Impact Profile score [28].

Advantages and disadvantages

Advantages

Liquid oxygen takes up less space than oxygen in its gas form, making it easier and lighter to carry around. Liquid oxygen tanks are safer compared to compressed gas cylinders because they are under lower pressure. Of the three current modes of delivery for domiciliary oxygen treatment, the most flexible and convenient source of home oxygen is the liquid oxygen system [29]. Light portable containers are refilled with liquid oxygen from the large stationary reservoir at the patient's home whenever necessary, giving the patient control over the refilling frequency [25, 30]. The base equipment provides oxygen for >11 days, and ambulatory oxygen in the portable canisters lasts 8–10 h [28, 31]. At a flow rate of 2 L·min⁻¹ of oxygen, this longer duration of oxygen supply in liquid form benefits patients with chronic respiratory disease who would otherwise be restricted to a maximum of 2 h of oxygen, thus limiting their time spent outdoors [18]. Modern liquid oxygen canisters are less cumbersome for the patient to carry than previously reported [32]: 3.5 kg when full *versus* 2.5 kg when empty [18] for the larger portable canisters, and even lighter for the smaller ones. When compared to gaseous oxygen, patients prefer the liquid oxygen system because the oxygen lasts longer, filling the canister is simpler, and the portable system is easier to carry due to a lighter weight [18]. However, portable oxygen concentrators are even lighter than liquid oxygen canisters because they do not require a storage reservoir of pressurised oxygen. Nonetheless, oxygen concentrators are less convenient for patients than liquid oxygen because they require internal batteries, automobile adaptors or standard electricity, and this need for a continuous power source could hinder patient mobility and independence.

Disadvantages

Oxygen tanks and liquid oxygen canisters are limited by a finite capacity defined by their size, whereas portable oxygen concentrators have no compressed tanks to exchange or refill given that they draw in ambient air directly from the surroundings, filter it instantly and deliver the approximately 93% pure oxygen directly to the patient through the nasal cannula. It is necessary to keep the large liquid

oxygen containers filled at home to replenish the smaller, portable tanks frequently. The recurring oxygen deliveries can get quite expensive. Another important point to remember is that the liquid oxygen constantly evaporates and needs to be used and resupplied by a professional service provider at least two to three times a month. Therefore, one of the main drawbacks for liquid oxygen therapy is the cost. In addition, the number of patients with impaired lung function wishing to travel by aeroplane is increasing, but aviation regulations prohibit liquid oxygen on commercial aircraft [33].

Cost

Compared with oxygen concentrator treatment, long-term liquid oxygen therapy is about four times more expensive [28, 30]. In their Swedish study in 1998, ANDERSSON *et al.* [28] found that the average total cost per patient over a 6-month period was USD 1310 for the concentrator group *versus* USD 4950 for the liquid oxygen group. There is a high delivery/service cost associated with refilling the liquid oxygen stationary systems at a set frequency, contingent on the oxygen flow setting and the unit's size [25]. In addition, other associated costs include electricity, acquisition costs and metering gas to the patient [25].

Oxygen delivery systems

Oxygen delivery systems are categorised into low-flow and high-flow systems. Low-flow systems provide lower oxygen flow than the actual inspiratory flow (~30 L·min⁻¹). When the patient inspires, the oxygen is diluted with room air, and the degree of dilution depends on the inspiratory flows. Therefore, these oxygen delivery systems do not allow for accurate calculation of the inspiratory oxygen fraction (F_{iO_2}). High-flow oxygen delivery systems provide higher oxygen flows and the F_{iO_2} is stable and is not affected by the patient's type of breathing.

Low-flow oxygen delivery systems

Nasal cannula

A nasal cannula is the most common oxygen delivery system, used for mild hypoxia (figure 4a). It delivers oxygen into the nasopharyngeal space and can be set to deliver between 1 and 6 L·min⁻¹ (24–40% F_{iO_2}) (table 2). F_{iO_2} increases by approximately 4% with each litre of oxygen per minute. Nasal cannulae are widely used in domiciliary oxygen devices. An oxygen flow >6 L·min⁻¹ should be avoided as it can dry the nasal mucosa and can disturb sleeping patterns [34, 35]. A nasal cannula is convenient as the patient can talk and eat while receiving oxygen, and it is easy to use. However,

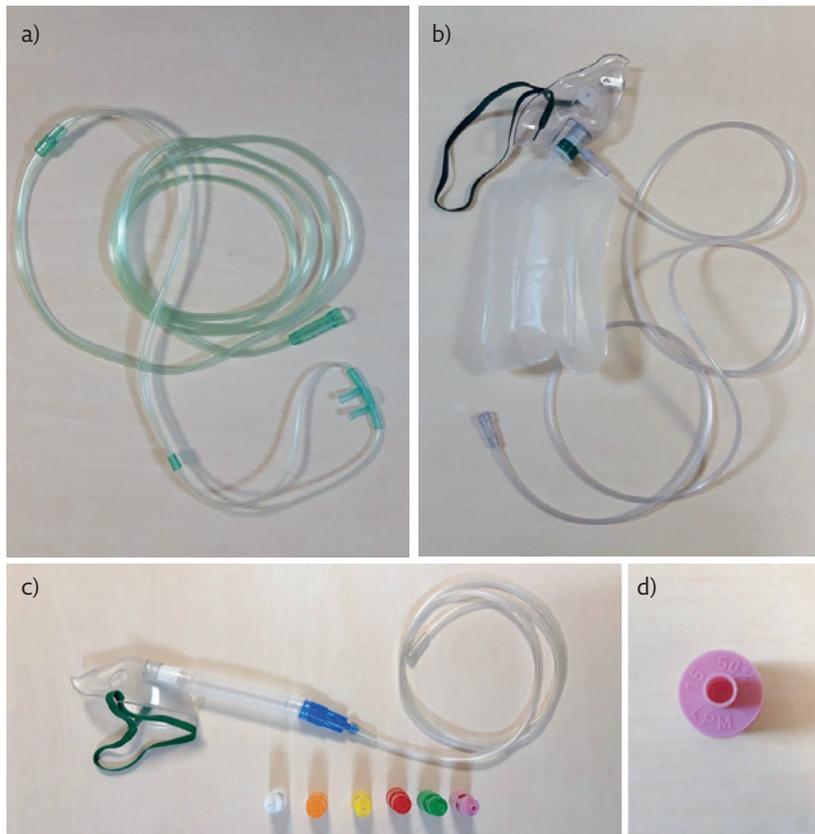


Figure 4 a) Nasal cannula. b) Non-rebreather mask. c) Venturi mask with different sized ports to change the F_{IO_2} delivered (24–50%). d) F_{IO_2} and oxygen flow are clearly stated on the bottom of each port.

Table 2 F_{IO_2} and oxygen flow delivered via nasal cannulae

| F_{IO_2} % | Flow $L \cdot \text{min}^{-1}$ |
|--------------|--------------------------------|
| 24–28 | 1–2 |
| 30–35 | 3–4 |
| 38–44 | 5–6 |

it can be easily dislodged and is not as effective in patients with deviated septum or polyps.

Simple face mask

A simple face mask can be set to deliver between 5 and 10 $L \cdot \text{min}^{-1}$ (35–55% F_{IO_2}) and is indicated when a moderate amount of oxygen is needed. It fits over the patient's mouth and nose, and has side exhalation ports through which the patient exhales carbon dioxide. Humidified air may be added if the oxygen concentrations are causing nasal mucosa dryness. The mask's efficiency relies on how well it fits. Eating and drinking can be difficult with the mask on and it can be confining for some patients, who may feel claustrophobic with the mask on [34, 35].

Non-rebreather mask

A non-rebreather mask is a low-flow device with high F_{IO_2} . It uses a reservoir bag (~1000 mL) to deliver a higher concentration of oxygen (figure 4b). A one-way valve between the mask and the reservoir bag prevents the patient from inhaling expired air. It can be set to deliver between 10 and 15 $L \cdot \text{min}^{-1}$ (80–95% oxygen). Oxygen flow $<10 L \cdot \text{min}^{-1}$ can cause the bag to completely collapse during inspiration. F_{IO_2} depends on the patient's pattern of breathing. This mask is useful in severely hypoxic patients who are ventilating well, but it carries the risk of carbon dioxide retention and aspiration in case of vomiting [34, 35].

Transtracheal oxygen catheter

Transtracheal oxygen catheters (TTOCs) can be effective in palliating breathlessness and hypoxaemia. The TTOC delivers oxygen directly into the trachea and it is inserted percutaneously into the trachea using Seldinger technique. However, TTOC placement has not gained widespread popularity as only a few physicians are trained to insert the TTOC or manage patients with it, and there is also a widespread reservation towards performing this invasive procedure on hypoxaemic, elderly, frail patients [36].

Oxygen flow through a TTOC ranges between 0.5 and 4 $L \cdot \text{min}^{-1}$. Oxygen delivery by TTOC bypasses the anatomical "dead space" in the upper airways and mouth, allowing oxygen to pass directly into the trachea. This reduces the overall oxygen needed during rest and with exercise.

High-flow oxygen delivery systems

Rebreather mask

Unlike the non-rebreather mask, there is no one-way valve between the rebreather mask and the reservoir bag and the inspired oxygen and expired air are collected in the reservoir bag.

Venturi mask

A Venturi mask is a high-flow device that allows precise measurement of F_{IO_2} delivered. It consists of a bottle of sterile water, corrugated tubing, air/oxygen ratio nebuliser system, a drainage bag, and a mask (*e.g.* aerosol face mask, tracheostomy mask, T-piece, a face tent). The oxygen flow exceeds the patient's peak expiratory flow. Therefore, it is unlikely for the patient to breathe in air from the room. A Venturi mask utilises different sized ports to change the F_{IO_2} delivered (24–50%) (figure 4c). The F_{IO_2} and oxygen flow are clearly stated on the bottom of each port (figure 4d). It does not dry mucous membranes, but it is confining for some patients, and it interferes with talking and eating. It is particularly useful in COPD patients, where precise oxygen delivery is crucial [34, 35].

High-flow nasal cannula

A high-flow nasal cannula consists of a flow generator, an air-oxygen blender, a humidifier and a nasal cannula. The flow generator can provide gas flow up to 60 L·min⁻¹, and the blender escalates F_{iO_2} up to 100% while the humidifier saturates the gas mixture (at 31–37°C). The heated humidified oxygen is delivered to a wide-bore nasal prong. The flow rate and F_{iO_2} can be independently titrated based on the patient's flow and F_{iO_2} requirements. Overall, high flows and humidification improve functional residual capacity and mucociliary

clearance of secretions, and thereby they reduce the work of breathing [34, 35].

Conclusions

Appropriate selection of oxygen devices and delivery systems depends on the degree of hypoxaemia, the existing evidence for the patient's underlying diagnosis and patient preference. Respiratory physicians should have a consolidated knowledge of all devices and systems to devise proper and individualised patient-based plans for oxygen therapy.

Affiliations

Georgia Hardavella¹, Ioannis Karampinis², Armin Frille^{3,4}, Katherina Sreter⁵, Ilona Rousalova⁶

¹10th Dept of Respiratory Medicine, Athens Chest Diseases Hospital "Sotiria", Athens, Greece. ²Dept of Thoracic Surgery, General Hospital "Sismanogleio", Athens, Greece. ³Dept of Respiratory Medicine, University of Leipzig, Leipzig, Germany. ⁴Integrated Research and Treatment Center (IFB) Adiposity Diseases, University Medical Center Leipzig, Leipzig, Germany. ⁵The Royal Marsden, NHS Foundation Trust, London, UK. ⁶1st Dept of Tuberculosis and Respiratory Diseases, General University Hospital and First Faculty of Medicine, Charles University, Prague, Czech Republic.

Acknowledgements

For this contribution, A. Frille was supported by the Federal Ministry of Education and Research (BMBF), Germany, FKZ 01EO1501 (IFB Adiposity Diseases, MetaRot program). The authors would like to thank BETABET company for kindly agreeing for photos to be taken of their merchandise.

Conflict of interest

None declared.

References

- Nocturnal Oxygen Therapy Trial Group. Continuous or nocturnal oxygen therapy in hypoxemic chronic obstructive lung disease: a clinical trial. *Ann Intern Med* 1980; 93: 391–398.
- Medical Research Council Working Party. Long term domiciliary oxygen therapy in chronic hypoxic cor pulmonale complicating chronic bronchitis and emphysema. *Lancet* 1981; 317: 681–686.
- O'Driscoll BR, Howard LS, Earis J, et al. BTS guideline for oxygen use in adults in healthcare and emergency settings. *Thorax* 2017; 72: Suppl. 1, ii1–ii90.
- Meena M, Dixit R, Kewlani JP, et al. Home-based long-term oxygen therapy and oxygen conservation devices: An updated review. *Natl J Physiol Pharm Pharmacol* 2015; 4: 267–273.
- Franklin KA, Gustafson T, Ranstam J, et al. Survival and future need of long-term oxygen therapy for chronic obstructive pulmonary disease – gender differences. *Respir Med* 2007; 101: 1506–1511.
- Croxton TL, Bailey WC. Long-term oxygen treatment in chronic obstructive pulmonary disease: recommendations for future research: an NHLBI workshop report. *Am J Respir Crit Care Med* 2006; 174: 373–378.
- Stoller JK, Panos RJ, Krachman S, et al. Oxygen therapy for patients with COPD: current evidence and the long-term oxygen treatment trial. *Chest* 2010; 138: 179–187.
- Neri M, Melani AS, Miorelli AM, et al. Long-term oxygen therapy in chronic respiratory failure: a Multicenter Italian Study on Oxygen Therapy Adherence (MISOTA). *Respir Med* 2006; 100: 795–806.
- Melani AS, Sestini P, Rottoli P. Home oxygen therapy: re-thinking the role of devices. *Expert Rev Clin Pharmacol* 2018; 11: 279–289.
- Jackson M, Shneerson J. An evaluation of the use of concentrators for domiciliary oxygen supply for less than 8 h day⁻¹. *Respir Med* 1998; 92: 250–255.
- Diego Gonzalez EG, Mendez Lanza A, Mosquera Pestana JA. Ruidos y averias: factores determinantes en la aceptacion y comportamiento del concentrador de O₂. Proyecto Asturias [Noise and machine failures: determining factors in the acceptance and behavior of O₂ concentrator. The Asturias project]. *An Med Interna* 1996; 13: 430–433.
- Diaz Lobato S, Garcia Gonzalez JL, Alises SM. The debate on continuous home oxygen therapy. *Arch Bronconeumol* 2015; 51: 31–37.
- Grand View Research. Medical Oxygen Concentrators Market Size, Share & Trends Analysis Report By Product (Portable, Stationary), By Application (Non-homecare, Homecare), By Technology (Pulse Dose, Continuous Flow), And Segment Forecasts, 2019–2025. Report ID: 978-1-68038-457-4. www.grandviewresearch.com/industry-analysis/medical-oxygen-concentrators-market Date last updated: April 2019. Date last accessed: 12 April 2019.
- Hardinge M, Annandale J, Bourne S, et al. British Thoracic Society guidelines for home oxygen use in adults. *Thorax* 2015; 70: Suppl. 1, i1–i43.
- Magnussen H, Kirsten AM, Köhler D, et al. Leitlinien zur Langzeit-Sauerstofftherapie. Deutsche Gesellschaft für Pneumologie und Beatmungsmedizin e.V. [Guidelines for

- long-term oxygen therapy. German Society for Pneumology and Respiratory Medicine]. *Pneumologie* 2008; 62: 748-756.
16. Casaburi R, Porszasz J, Hecht A, *et al.* Influence of lightweight ambulatory oxygen on oxygen use and activity patterns of COPD patients receiving long-term oxygen therapy. *COPD* 2012; 9: 3-11.
 17. Strickland SL, Hogan TM, Hogan RG, *et al.* A randomized multi-arm repeated-measures prospective study of several modalities of portable oxygen delivery during assessment of functional exercise capacity. *Respir Care* 2009; 54: 344-349.
 18. Lock SH, Blower G, Prynne M, *et al.* Comparison of liquid and gaseous oxygen for domiciliary portable use. *Thorax* 1992; 47: 98-100.
 19. Petty TL. Historical highlights of long-term oxygen therapy. *Respir Care* 2000; 45: 29-36.
 20. Petty TL, Casabury R. Recommendations of the Fifth Oxygen Consensus Conference. *Respir Care* 2000; 45: 957-961.
 21. BOC, NHS. Liquid Oxygen Mother Unit/Portable Flask System: Equipment Guide. Manchester, BOC Healthcare, 2012. www.bochohomeoxygen.co.uk/en/images/406735_Healthcare_Liquid_Systems_Handbook_NHS_View_tcm1109-179233.pdf
 22. BOC. Liquid Medical Oxygen: Essential Safety Information. Medical Gas Data Sheet. Manchester, BOC Healthcare, 2013. www.boconline.co.uk/en/images/medical_liquid_oxygen_tcm410-55834.pdf
 23. Air Products. Liquid Oxygen. Allentown, Air Products and Chemicals Inc., 2015. www.airproducts.com/~media/files/pdf/company/safetygram-6.pdf
 24. McCoy RW. Liquid oxygen applications from hospital to home. *Home Pathways* 2005; 14: 32.
 25. McCoy RW. Options for home oxygen therapy equipment: storage and metering of oxygen in the home. *Respir Care* 2013; 58: 65-85.
 26. Pépin JL, Barjhoux CE, Deschaux C, *et al.* Long-term oxygen therapy at home. Compliance with medical prescription and effective use of therapy. ANTADIR Working Group on Oxygen Therapy. Association Nationale de Traitement à Domicile des Insuffisants Respiratoires. *Chest* 1996; 109: 1144-1150.
 27. Su CL, Lee CN, Chen HC, *et al.* Comparison of domiciliary oxygen using liquid oxygen and concentrator in northern Taiwan. *J Formos Med Assoc* 2014; 113: 23-32.
 28. Andersson A, Ström K, Brodin H, *et al.* Domiciliary liquid oxygen versus concentrator treatment in chronic hypoxaemia: a cost-utility analysis. *Eur Respir J* 1998; 12: 1284-1289.
 29. Gorecka D. Liquid oxygen, is it the gold standard? *Chron Respir Dis* 2005; 2: 181-182.
 30. Kacmarek RM. Delivery systems for long-term oxygen therapy. *Respir Care* 2000; 45: 84-92.
 31. Welch GH, Werinberg DE, Welch WP. The use of Medicare home health care services. *N Engl J Med* 1996; 335: 324-329.
 32. Leggett RJ, Flenley DC. Portable oxygen and exercise tolerance in patients with chronic hypoxic cor pulmonale. *Br Med J* 1977; 2: 84-86.
 33. Fischer R, Wanka ER, Einhaeupl F, *et al.* Comparison of portable oxygen concentrators in a simulated airplane environment. *Respir Med* 2013; 107: 147-149.
 34. Korupolu R, Gifford J, Needham DM. Early mobilization of critically ill patients: reducing neuromuscular complications after intensive care. *Contemp Crit Care* 2009; 6: 1-12.
 35. Bailey P, Thomsen GE, Spuhler VJ, *et al.* Early activity is feasible and safe in respiratory failure patients. *Crit Care Med* 2007; 35: 139-145.
 36. Christopher KL. Transtracheal oxygen catheters. *Clin Chest Med* 2003; 24: 489-510.